



WARNING!

Risk of Entrapment

There's a risk of entrapment or suffocation between mattress support, side rail and bed end.

- When using steel side rails, always make sure that the distance between the bed end and the side rails handle upper edge is less than 6 cm in the head end and more than 32 cm in the foot end of the bed.

CAUTION!

There is a risk of entrapment of fingers on assembly and operation of the side rail.



- Pay attention to your hands when using side rails.

User Instructions for Hospital Bed 3/4 Length Rails
Installation:




Place the U-formed side rail brackets onto the outer frame on the correct side of the bed. The Flat end of the rail should be at the head of the bed and swing towards the foot end when lowering. The flat end of the rail should be as far towards the head of the bed as possible to reduce the risk of entrapment. (fig. 1)

Locate the knob hanging down from the U-formed bracket at both ends of the rail. (fig 2) . Swing the knob up into place and tighten by turning clockwise. (fig. 3)

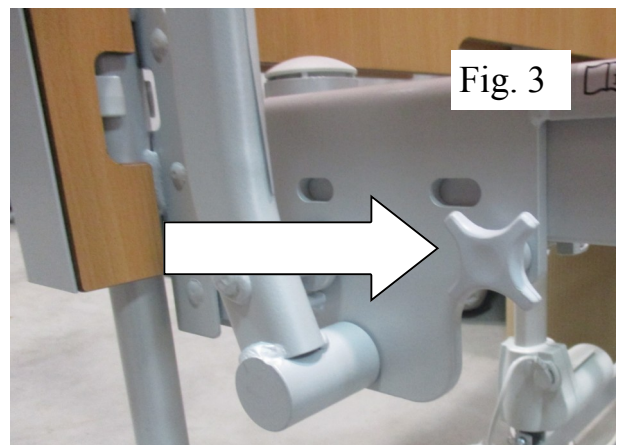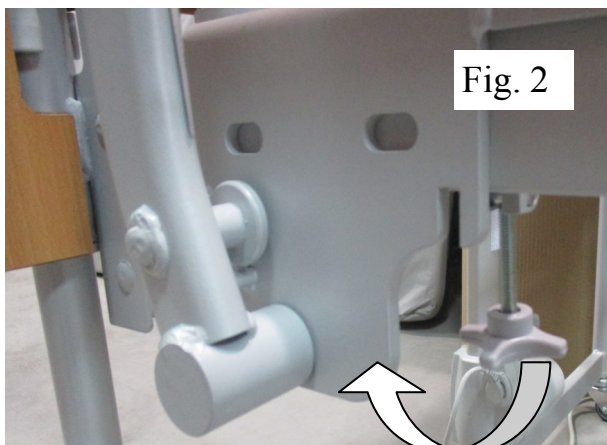

User Instructions for Hospital Bed 3/4 Length Rails

Operation:

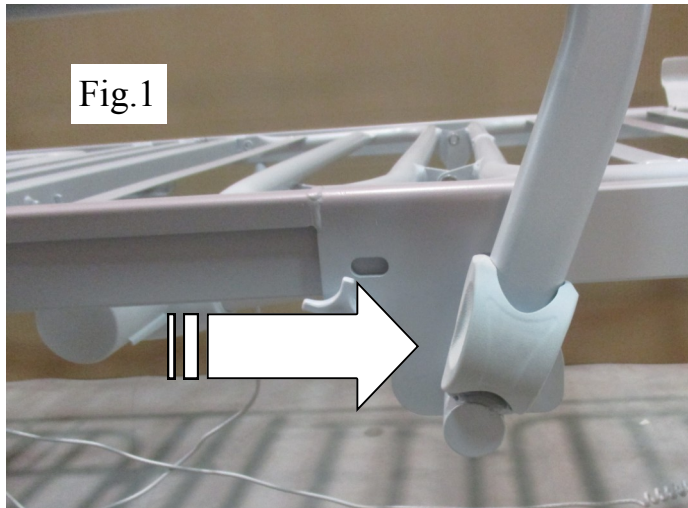



Folding down the side rail:

Locate the plastic release knob at the foot end of the rail. (fig. 1)

Pull the knob out and at the same time rotate the rail down and towards the foot end of the bed (fig. 2) until rail is in lowest position. (fig. 3)

Folding up the side rail:

Hold the top bar of the rail and pull up until it locks in place with a clicking sound.

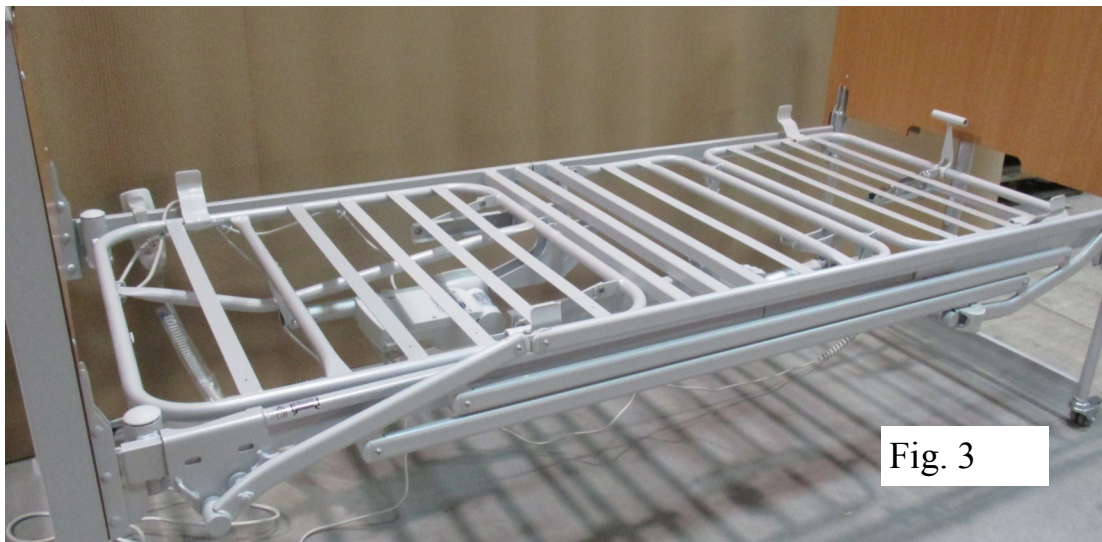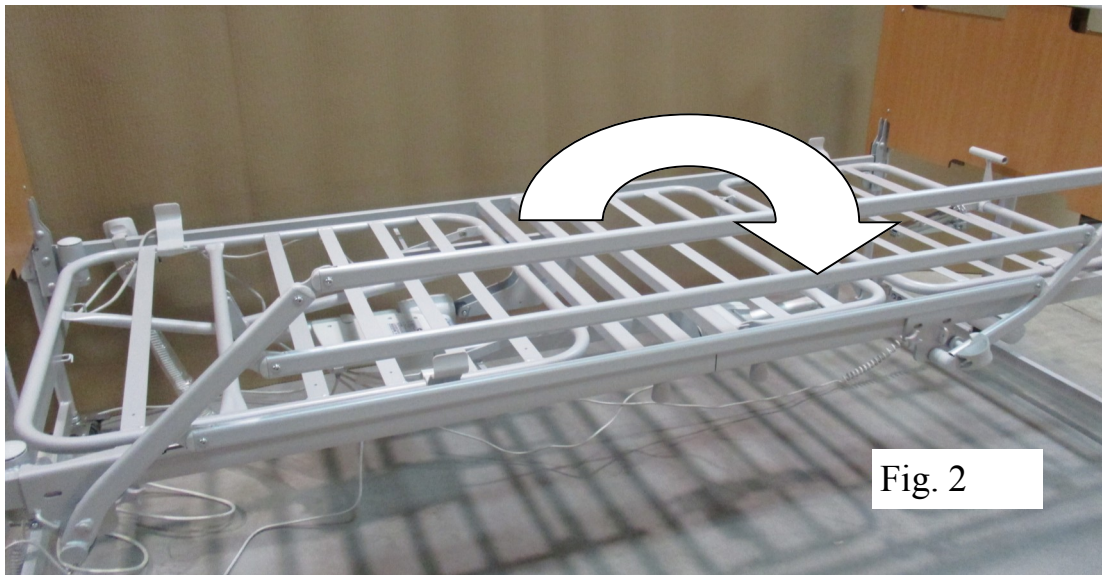

CAUTION!

If the side rail is not locked properly it can fall down.

- Pull/push the top bar of the side rail to ensure that the locking mechanism is properly engaged.